EUCAST EUROPEAN COMMITTEE ON ANTIMICROBIAL SUSCEPTIBILITY TESTING

European Society of Clinical Microbiology and Infectious Diseases

European Committee on Antimicrobial Susceptibility Testing

Routine and extended internal quality control for MIC determination and agar dilution for yeasts, moulds and dermatophytes as recommended by EUCAST

Version 6.0, valid from 2022-05-04

This document should be cited as: "The European Committee on Antimicrobial Susceptibility Testing. Routine and extended internal quality control for MIC determination and agar dilution for yeasts, moulds and dermatophytes as recommended by EUCAST. Version 6.0, 2022. http://www.eucast.org."

General	**Page**
Notes	1
Changes	2

Routine quality control	**Page**
Recommended strains for routine quality control	3
One-page Summary of MIC targets and ranges for yeast and mould testing	4
Candida krusei ATCC 6258	5
Candida parapsilosis ATCC 22019	6
Candida albicans CNM-CL F8555	7
Candida krusei CNM-CL 3403	8
Aspergillus fumigatus ATCC 204305	9
Aspergillus flavus ATCC 204304	10
Aspergillus flavus CNM-CM 1813	11
Aspergillus fumigatus SSI-4524	12
Aspergillus fumigatus SSI-5586	13
Trichophyton indotineae (prev. *Trichophyton interdigitale*) SSI-9363	14
Trichophyton rubrum SSI-7583	15
Aspergillus fumigatus DPL1035 homo/SSI-1794	16
Aspergillus fumigatus ATCC MYA-1163	17
Aspergillus fumigatus DPL32458	18
Aspergillus fumigatus DPL55985	19

Notes

Version 6.0, valid from 2022-05-04

1. In EUCAST quality control (QC) tables, both ranges and targets are listed. Repeat testing of EUCAST quality control strains should yield individual MIC values randomly distributed within the recommended ranges. If the number of tests is ≥10, the mode MIC should be the target value.

2. Ranges and targets are established by EUCAST.

3. EUCAST quality control strains for routine QC are used to monitor the entire test performance (material, inoculum, incubation, reading etc). At least 2 quality control strains with different target MICs should be tested at regular intervals, or if panels are used irregularly with every panel set up for clinical use or research purposes. Mould QC strains should always be included for antifungal susceptibility testing of mould, specially when using the resistance agar-screening methods (E.Def 10.2).

4. QC ranges are presented both as a one-page summary and in separate tables for each strain. Both tables contain the same data.

5. For information about the reference methods for susceptibility testing of yeast and moulds see "Methods in antifungal susceptibility testing of yeasts E.Def 7.3.2", "Methods in antifungal susceptibility testing of moulds E.Def 9.4 and 10.2", and "Methods in antifungal susceptibility testing of dermatophytes E.Def 11.0", respectively.

6. Abreviations: ATCC: American Type Culture Collection. CNM-CL: Yeast collection of the Spanish National Centre of Microbiology. SSI: Statens Serum Institute. DPL: David Perlin.

7. Strain availability information: The QC strains (except the ATCC strains) are deposited in the Culture Collection University of Gothenburg https://www.ccug.se/ from where they are available.

8. *A. fumigatus* SSI-4524: a QC strain harbouring TR_{34}/L98H substitution for quality control of azole-containing agar plates.

9. *A. fumigatus* SSI-5586: a QC harbouring G54W substitution for quality control of azole-containing agar plates.

10. *T. indotineae* (previously classified as *T. interdigitale*) SSI-9363: a wild type strain.

11. *T. rubrum* SSI-7583: a wildtype strain.

12. *A. fumigatus* DPL1035 homo/SSI-1794.

Changes from previous version

Version 6.0, valid from 2022-05-04	**Changes** Cells containing a change or an addition from EUCAST QC Tables v. 5.0 are marked yellow (Format changes are not marked yellow).
1. Notes	The new species name (*T. indotineae*) for the "Indian" *T. interdigitale* has been specified. Info on abreviations and strain availability have been added. Four new QC strains have been added.
3. Routine QC	The new species name (*T. indotineae*) for the "Indian" *T. interdigitale* has been specified. The new QC strain for echinocandin agar screening has been included.
4. Summary Antifungals QCs	The new species name *(T. indotineae*) for the "Indian" *T. interdigitale* has been specified. And information on interpretation of QC strains on echinocandin agar included.
9. ATCC 204305	Information on colony morphology for this QC strain on echinocandin resistance screening agar has been provided. Reference to E.Def 9.3.2 have been revised to 9.4
10. ATCC 204304	Reference to E.Def 9.3.2 have been revised to 9.4
11. CNM-CM 1813	Reference to E.Def 9.3.2 have been revised to 9.4
14. SSI-9363	The strain originating from India was previously classified as *T. interdigitale* and has been submitted to databases as such. However it has recently been reclassified to a new species *Trichophyton indotineae* which is related to both *T. interdigitale* and *T. rubrum.* This species is particularly prevalent in India and other Asian countries.
16. DPL1035 homo/SSI-1794	A new QC strain suitable for the echinocandin agar screening method: *A. fumigatus* DPL1035 homo/SSI-1794 has been added.
17. ATCC MYA-1163	A new QC strain suitable for the echinocandin agar screening method: *A. fumigatus* ATCC MYA-1163 has been added.
18. DPL32458	A new QC strain suitable for the echinocandin agar screening method: *A. fumigatus* DPL32458 has been added.
19. DPL55985	A new QC strain suitable for the echinocandin agar screening method: *A. fumigatus* DP55985 has been added.

EUCAST EUROPEAN COMMITTEE ON ANTIMICROBIAL SUSCEPTIBILITY TESTING
European Society of Clinical Microbiology and Infectious Diseases

Version 6.0, valid from 2022-05-04

Routine quality control

Candida krusei ATCC 6258
Candida parapsilosis ATCC 22019
Candida albicans CNM-CL F8555
Candida krusei CNM-CL 3403
Aspergillus fumigatus ATCC 204305
Aspergillus flavus ATCC 204304
Aspergillus flavus CNM-CM 1813
Aspergillus fumigatus SSI-4524
Aspergillus fumigatus SSI-5586
Trichophyton indotineae (prev. *Trichophyton interdigitale*) SSI-9363
Trichophyton rubrum SSI-7583
Aspergillus fumigatus DPL1035 homo/SSI-1794

European Subcommittee on Antifungal Susceptibility Testing (EUCAST AFST)

Routine and extended internal quality control for antifungal susceptibility as recommended by EUCAST

Version 6.0, valid from 2022

This document should be cited as: "The European Committee on Antimicrobial Susceptibility Testing. Routine and extended internal quality control for MIC determination and agar dilution for yeasts, moulds and dermatophytes as recommended by EUCAST. Version 6.0, 2022. http://www.eucast.org."

QC strains	Drug MICs (mg/L)																			
	Amphotericin B		Anidulafungin		Fluconazole		5-FC		Isavuconazole		Itraconazole		Micafungin		Voriconazole		Posaconazole		Terbinafine	
	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range	Target	Range
Candida krusei ATCC 6258	0.25-0.5	0.125-1	0.03	0.016-0.06	32	16-64	2	1-4	0.03	0.016-0.06	0.06	0.03-0.125	0.06	0.03-0.125	0.06-0.125	0.03-0.25	0.03	0.016-0.06	-	-
Candida parapsilosis ATCC 22019	0.25-0.5	0.125-1	0.5	0.25-1	1	0.5-2	0.25	0.125-0.5	0.016	0.008-0.03	0.06	0.03-0.125	1	0.5-2	0.03	0.016-0.06	0.03	0.016-0.06	-	-
Candida albicans CNM-CL F8555	0.125-0.25	0.06-0.5	-	-	64	32-128	0.125	0.06-0.25	-	-	0.5	0.25-1	-	-	1	0.5-2	0.25	0.125-0.5	-	-
Candida krusei CNM-CL 3403	0.5	0.25-1	-	-	32	16-64	4	2-8	-	-	0.25	0.125-0.5	-	-	0.25	0.125-0.5	0.125	0.06-0.25	-	-
Aspergillus fumigatus ATCC 204305	0.5	0.25-1	-	-	-	-	-	-	-	-	0.25	0.125-0.5	-	-	0.5	0.25-1	0.06-0.125	0.03-0.25	-	-
Aspergillus flavus ATCC 204304	1	0.5-2	-	-	-	-	-	-	-	-	0.25	0.125-0.5	-	-	1	0.5-2	0.25	0.125-0.5	0.5	0.25-1
Aspergillus flavus CNM-CM 1813	2	1-4	-	-	-	-	-	-	-	-	0.25	0.125-0.5	-	-	1	0.5-2	0.25	0.125-0.5	0.5	0.25-1
Trichophyton indotineae SSI-9363*#											[0.06]	[0.03-0.25]			[0.25]	[0.125-1]			[0.016]	[0.016-0.06]
Trichophyton rubrum SSI-7583*											[0.016]	[0.008-0.03]			[0.03]	[0.008-0.03]			[0.016]	[0.008-0.03]

* Targets and ranges for *Trichophyton* isolates are tentative hence in brackets. # *T. indotineae* was previously regarded as a variant of *T. interdigitale*

E.Def 10.2 Growth scoring and interpretation on azole and echinocandin screening agar plates for EUCAST recommended QC strains (two days of incubation)

Design of 4-well azole plate:

Itraconazole (4 mg/L)	Voriconazole (2 mg/L)
Posaconazole (0.5 mg/L)	Growth control (-)

Scores for QC strains on azole agar (48 h):

***Aspergillus fumigatus* SSI-4524**

2-3 0.5-2

0-1 3

***Aspergillus fumigatus* SSI-5586**

2-3 0

2-3 3

Score definition Azole agar: **0**: no visible growth; **0.5**: 1-5 tiny colonies; **1**: weak/minimal growth (either as >5 tiny colonies or confluent weak growth where the azole agar has been inoculated (covering ≤ half the well); **2**: clearly visible growth with hyphal extension but not covering the entire well (and less than the control well); **3**: un-inhibited prominent growth covering the majority of the well and similar to that in the control well.

Design of 4-well echinocandin plate:

	Anidulafungin (0.25 mg/L)
Micafungin (0.125 mg/L)	Growth control (-)

Reading QC strains on echinocandin agar (48 h):

***Aspergillus fumigatus* ATCC 204305**

Disk like*

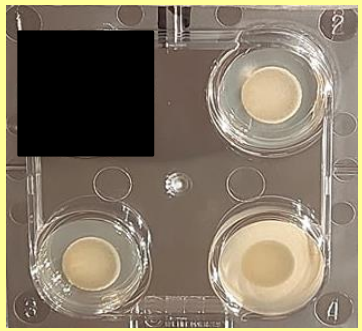

Disk like* fluffy extensively radiating hyphae

***Aspergillus fumigatus* DPL103/SSI-1794**

fluffy radiating hyphae

fluffy radiating hyphae fluffy radiating hyphae

***Disk like morphology on echinocandin agar (discreete radiating hyphae but much less than in control well)

Additional QC strains for echinocandin agar screening are shown in page 17-19

Candida krusei ATCC 6258[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 7.3.2 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	0.25-0.5	0.125-1
Anidulafungin	0.03	0.016-0.06
Caspofungin	NA[c]	NA[c]
Fluconazole	32	16-64
Flucytosine	2	1-4
Isavuconazole	0.03	0.016-0.06
Itraconazole	0.06	0.03-0.125
Micafungin	0.06	0.03-0.125
Voriconazole	0.06-0.125	0.03-0.25
Posaconazole	0.03	0.016-0.06

[a] ATCC: American Type Culture Collection.

[b] *Candida* QC strains requires MIC reading in a spectrophotometer after one day of incubation.

[c] Not available.

Candida parapsilosis ATCC 22019[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 7.3.2 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	0.25-0.5	0.125-1.0
Anidulafungin	0.5	0.25-1.0
Caspofungin	NA[c]	NA[c]
Fluconazole	1	0.5-2
Flucytosine	0.25	0.125-0.5
Isavuconazole	0.016	0.008-0.03
Itraconazole	0.06	0.03-0.125
Micafungin	1	0.5-2
Voriconazole	0.03	0.016-0.06
Posaconazole	0.03	0.016-0.06

[a] ATCC: American Type Culture Collection.

[b] *Candida* QC strains requires MIC reading in a spectrophotometer after one day of incubation.

[c] Not available.

Candida albicans CNM-CL F8555[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 7.3.2 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	**Range**
Amphotericin B	0.125-0.25	0.06-0.5
Anidulafungin	NA[c]	NA[c]
Caspofungin	NA[c]	NA[c]
Fluconazole	64	32-128
Flucytosine	0.125	0.06-0.25
Isavuconazole	NA[c]	NA[c]
Itraconazole	0.5	0.25-1
Micafungin	NA[c]	NA[c]
Voriconazole	1	0.5-2
Posaconazole	0.25	0.125-0.5

[a] CNM-CL: Yeast collection of the Spanish National Centre of Microbiology. The QC strain is deposited in the Culture Collection University of Gothenburg https://www.ccug.se/ from where will be available.

[b] *Candida* QC strains requires MIC reading in a spectrophotometer after one day of incubation.

[c] Not available.

Candida krusei CNM-CL 3403[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 7.3.2 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	0.5	0.25-1
Anidulafungin	NA[c]	NA[c]
Caspofungin	NA[c]	NA[c]
Fluconazole	32	16-64
Flucytosine	4	2-8
Isavuconazole	NA[c]	NA[c]
Itraconazole	0.25	0.125-0.5
Micafungin	NA[c]	NA[c]
Voriconazole	0.25	0.125-0.5
Posaconazole	0.125	0.06-0.25

[a] CNM-CL: Yeast collection of the Spanish National Centre of Microbiology. The QC strain is deposited in the Culture Collection University of Gothenburg https://www.ccug.se/ from where will be available.

[b] *Candida* QC strains requires MIC reading in a spectrophotometer after one day of incubation.

[c] Not available.

Aspergillus fumigatus ATCC 204305[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 9.4 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	0.5	0.25-1
Anidulafungin	NA[c]	NA[c]
Caspofungin	NA[c]	NA[c]
Fluconazole	NA[c]	NA[c]
Flucytosine	NA[c]	NA[c]
Isavuconazole	NA[c]	NA[c]
Itraconazole	0.25	0.125-0.5
Micafungin	NA[c]	NA[c]
Voriconazole	0.5	0.25-1
Posaconazole	0.06-0.125	0.03-0.25

[a] ATCC: American Type Culture Collection.

[b] *Aspergillus* QC strains should be read visually at a no growth inhibition endpoint after 2 days of incubation.

[c] Not available.

See EUCAST E.Def 10.2 for echinocandin screening agar method

QC strain which is a phenotypically wild type for echinocandins
Well 2 anidulafungin (0.25 mg/L), well 3 micafungin (0.125 mg/L), and well 4 drug free control well.

Reading criteria

Echinocandin wild-type phenotype:
Aspergillus strains with wild-type phenotype grow with a dense disk like appearance on echinocandin agars without the typical fluffy radiation halo around the main colony found only on drug free agar.

Reverse 24 h

Reverse 48 h

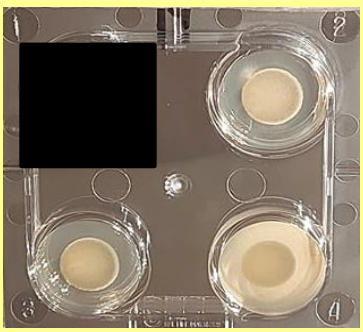

Aspergillus flavus ATCC 204304[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 9.4 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	1	0.5-2
Anidulafungin	NA[c]	NA[c]
Caspofungin	NA[c]	NA[c]
Fluconazole	NA[c]	NA[c]
Flucytosine	NA[c]	NA[c]
Isavuconazole	NA[c]	NA[c]
Itraconazole	0.25	0.125-0.5
Micafungin	NA[c]	NA[c]
Terbinafine	0.5	0.25-1
Voriconazole	1	0.5-2
Posaconazole	0.25	0.125-0.5

[a] ATCC: American Type Culture Collection.

[b] *Aspergillus* QC strains should be read visually at a no growth inhibition endpoint after 2 days of incubation.

[c] Not available.

Aspergillus flavus CNM-CM 1813[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 9.4 for MIC methodology

Antimicrobial agent	MIC[b] (mg/L)	
	Target	Range
Amphotericin B	2	1-4
Anidulafungin	NA[c]	NA[c]
Caspofungin	NA[c]	NA[c]
Fluconazole	NA[c]	NA[c]
Flucytosine	NA[c]	NA[c]
Isavuconazole	NA[c]	NA[c]
Itraconazole	0.25	0.125-0.5
Micafungin	NA[c]	NA[c]
Terbinafine	0.5	0.25-1
Voriconazole	1	0.5-2
Posaconazole	0.25	0.125-0.5

[a] CNM-CM: Spanish National Centre for Microbiology, Filamentous Fungi Culture Collection. The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where will be available.

[b] *Aspergillus* QC strains should be read visually at a no growth inhibition endpoint after 2 days of incubation.

[c] Not available.

A. fumigatus SSI-4524 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for azole screening test

QC strain harbouring TR34/L98H substitution for quality control of azole-containing agar plates.

Well 1 (itraconazole 4 mg/L), well 2 (voriconazole 2 mg/L), well 3 (posaconazole 0.5 mg/L), and well 4 (drug free control well).

Score definition
0: no visible growth;
0.5: 1-5 tiny colonies;
1: weak/minimal growth (either as >5 tiny colonies or confluent weak growth where the agar has been inoculated (covering ≤ half the well));
2: clearly visible growth with hyphal extension but not covering the entire well (and less than the control well);
3: un-inhibited prominent growth covering the majority of the well and similar to that in the control well.

2-3	0.5-2
0-1	3

[a] SSI: Statens Serum Institut, Copenhagen, Denmark
The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where it is available.

A. fumigatus SSI-5586 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for azole screening test

QC strain harbouring G54W substitution for quality control of azole-containing agar plates.

Well 1 (itraconazole 4 mg/L), well 2 (voriconazole 2 mg/L), well 3 (posaconazole 0.5 mg/L), and well 4 (drug free control well).

Score definition
0: no visible growth;
0.5: 1-5 tiny colonies;
1: weak/minimal growth (either as >5 tiny colonies or confluent weak growth where the agar has been inoculated (covering ≤ half the well));
2: clearly visible growth with hyphal extension but not covering the entire well (and less than the control well);
3: un-inhibited prominent growth covering the majority of the well and similar to that in the control well.

2-3	0
2-3	3

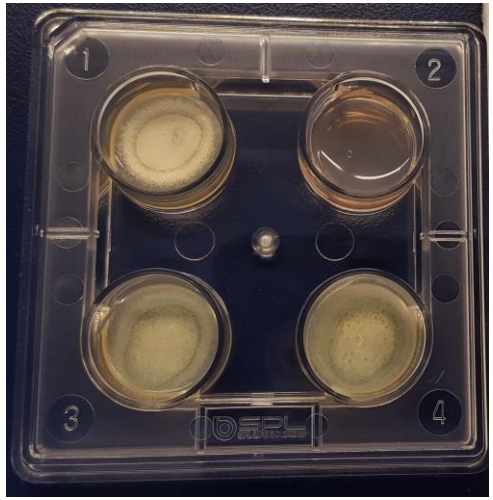

[a] SSI: Statens Serum Institut, Copenhagen, Denmark
The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where it is available

Trichophyton indotineae (prev. *Trichophyton interdigitale*) SSI-9363[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 11.0 for MIC methodology

Antimicrobial agent	MIC (mg/L)	
	Target	Range
Amorolfine	(0.125-0.25)	(0.03-0.25)
Amphotericin B	NA[b]	NA[b]
Anidulafungin	NA[b]	NA[b]
Caspofungin	NA[b]	NA[b]
Fluconazole	NA[b]	NA[b]
Flucytosine	NA[b]	NA[b]
Isavuconazole	NA[b]	NA[b]
Itraconazole	0.06	(0.03-0.25)
Micafungin	NA[b]	NA[b]
Terbinafine	(0.016)	(0.016-0.06)
Voriconazole	(0.25)	(0.125-1)
Posaconazole	NA[b]	NA[b]

[a] SSI: Statens Serum Institut, Copenhagen, Denmark. The QC strain is deposited in the Culture Collection University of Gothenburg https://www.ccug.se/ from where it is available.

[c] Not available.

Values indicated in brackets () are tentative

Trichophyton rubrum SSI-7583[a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 11.0 for MIC methodology

Antimicrobial agent	MIC (mg/L)	
	Target	Range
Amorolfine	(0.125)	(0.03-0.125)
Amphotericin B	NA[b]	NA[b]
Anidulafungin	NA[b]	NA[b]
Caspofungin	NA[b]	NA[b]
Fluconazole	NA[b]	NA[b]
Flucytosine	NA[b]	NA[b]
Isavuconazole	NA[b]	NA[b]
Itraconazole	(0.016)	(0.008-0.03)
Micafungin	NA[b]	NA[b]
Terbinafine	(0.016)	(0.008-0.03)
Voriconazole	(0.03)	(0.008-0.03)
Posaconazole	NA[b]	NA[b]

[a] SSI: Statens Serum Institut, Copenhagen, Denmark. The QC strain is deposited in the Culture Collection University of Gothenburg https://www.ccug.se/ from where it ise available.

[c] Not available.
Values indicated in brackets () are tentative

A. fumigatus DPL1035 homo/SSI-1794 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for echinocandin screening test

QC strain harbouring a substitution for quality control of echinocandin-containing agar plates. The strain is laboratory engeneered and derives from David Perlin's laboratory. Well 2 anidulafungin (0.25 mg/L), well 3 micafungin (0.125 mg/L), and well 4 drug free control well.

Reading criteria

Echinocandin non wild-type phenotype with anidulafungin and micafungin EUCAST MEC 16 and 4 mg/L, respectively:
The candin strain with non wild-type phenotype produce the fluffy radiating ring both on drug free and drug containing agars after 48h incubation. Similar growth between drug-free and drug-containing wells is observed after 24h.

Echinocandin wild-type phenotype (see QC ATCC MYA-1163 and QC ATCC 204305):
Aspergillus wildtype strains grow with a dense disk like appearence on candin agars without the typical fluffy radiation halo around the main colony found only on drug free agar.

	24h incubation	**48h incubation**
Front:		
Reverse: read in a mirror	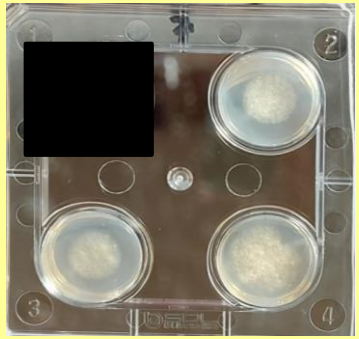	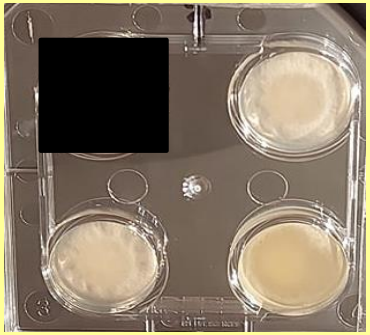

[a] SSI: Statens Serum Institut, Copenhagen, Denmark
The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where it is available

A. fumigatus ATCC MYA-1163 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for echinocandin screening test

QC strain which is a phenotypically wild type for echinocandins

Well 2 anidulafungin (0.25 mg/L), well 3 micafungin (0.125 mg/L), and well 4 drug free control well.

Echinocandin wild-type phenotype:
Aspergillus strains with wild-type phneotype grow with a dense disk like appearance on echinocandin agars without the typical fluffy radiation halo around the main colony found only on drug free agar.

	24h incubation	**48h incubation**
Front:		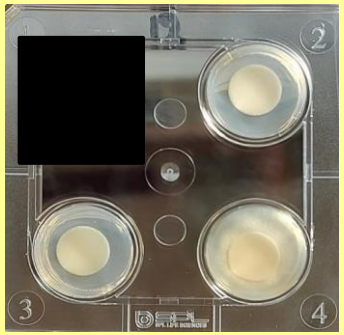
Reverse: read in a mirror	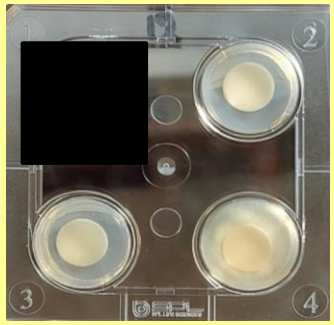	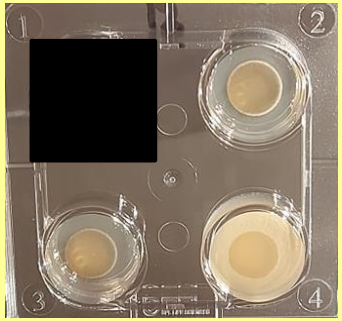

[a] The QC strain is available from the www.ATCC.org, and from the Culture Collection Universisy of Gothenburg https://www.ccug.se/

A. fumigatus AFM32458 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for echinocandin screening test

Strain deriving from a patient failing echinocandin therapy. Suitable as a QC strain for echinocandin-containing agar plates. The strain derives from David Denning's laboratory.
Well 2 anidulafungin (0.25 mg/L), well 3 micafungin (0.125 mg/L), and well 4 drug free control well.

Reading criteria

Echinocandin non wild-type phenotype with anidulafungin and micafungin EUCAST MEC 16 and 8 mg/L, respectively:
The candin strain with non wild-type phenotype produce the fluffy radiating ring both on drug free and drug containing agars after 48h incubation. Similar growth between drug-free and drug-containing wells is observed after 24h.

Echinocandin WT (see QC ATCC MYA-1163 and QC ATCC 204305):
Aspergillus WT strains grow with a dense disk like appearence on candin agars without the typical fluffy radiation halo around the main colony found only on drug free agar.

	24 h incubation	48 h incubation
Front:	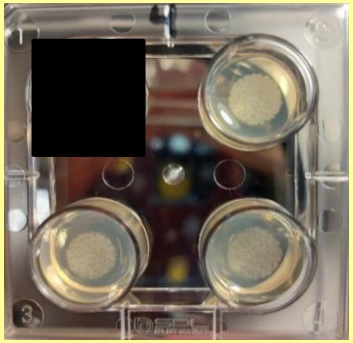	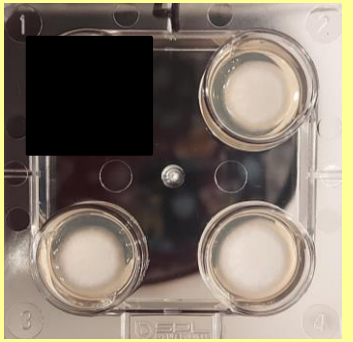
Reverse: read in a mirror	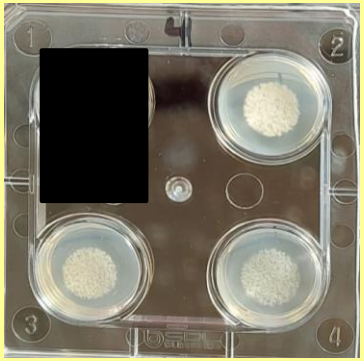	

[a] The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where it is available

A. fumigatus DPL55985 [a]

Version 6.0, valid from 2022-05-04

See EUCAST E.Def 10.2 for echinocandin screening test

Echinocandin resistant laboratory selected strain. Suitable as a QC strain for echinocandin-containing agar plates. The strain derives from David Perlin's laboratory.

Well 2 anidulafungin (0.25 mg/L), well 3 micafungin (0.125 mg/L), and well 4 drug free control well.

Reading criteria

Echinocandin non wild-type phenotype (anidulafungin and micafungin EUCAST MEC 4 and 8 mg/L, respectively)
The strain produce a comparable fluffy radiating ring both on drug free and drug containing agars after 48h incubation. Similar colony morphology comparing drug-free and drug-containing wells is also observed after 24h.

Echinocandin S (see QC ATCC MYA-1163 and QC ATCC 204305):
Aspergillus wildtype strains grow with a dense disk like appearence on candin agars without the typical fluffy radiation halo around the main colony found only on drug free agar.

Front 24 h incubation

Front 48 h incubation

Reverse 48 h incubation
(read in a mirror)

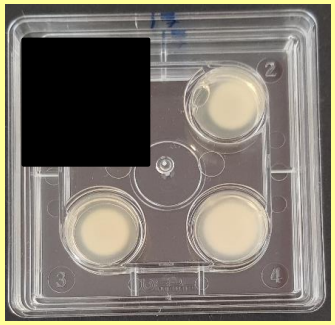

[a] The QC strain is deposited in the Culture Collection Universisy of Gothenburg https://www.ccug.se/ from where it is available